



For a translated user guide, please scan the QR code or visit the website [www.allflex.global/rapidmatic-evo](http://www.allflex.global/rapidmatic-evo)

**Allflex New Zealand Ltd**  
17 El Prado Drive  
Palmerston North  
06 3567199  
[www.allflex.co.nz](http://www.allflex.co.nz)

**Allflex Australia Pty Ltd**  
185 Queensport Road  
Murarrie QLD 4172  
1300 138 247  
[www.allflex.com.au](http://www.allflex.com.au)



# RapIDMatic Evo Applicator


For the application of Allflex RapID Evo tags only

Copyright © 2024 Merck & Co., Inc., Rahway, NJ, USA and its affiliates.  
All rights reserved. AH1-NON-240600001







1  
Ensure loader/cutter is in the locked position (at front of applicator).

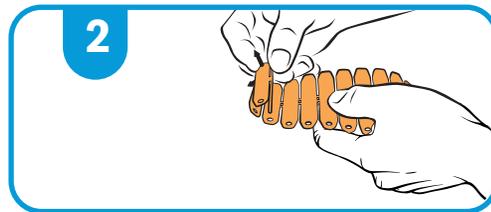


2  
Roll RapID Evo Tags towards you firmly. Bias the pins outwards to avoid jamming.

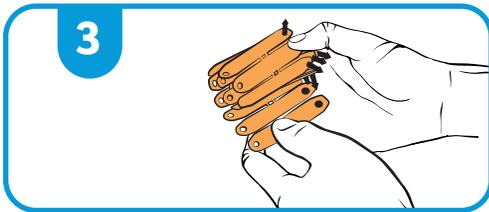

3  
Leave the last two RapID Evo Tags Unrolled.

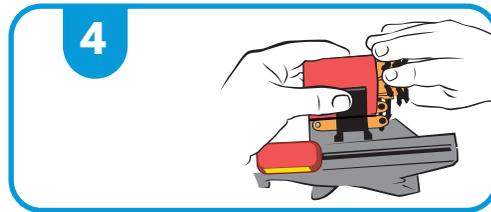



4  
Load into drum.

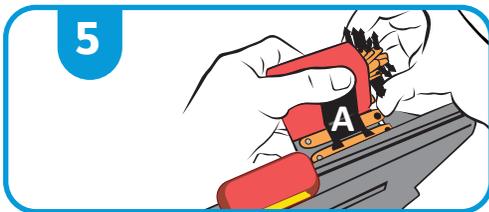


5  
Depress the clamp (A) firmly. Slide tags out until location lugs are between first and second tags.




6  
Pull trigger to move tag into the Load position.

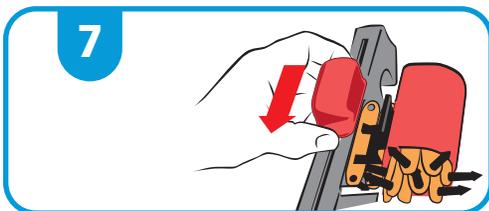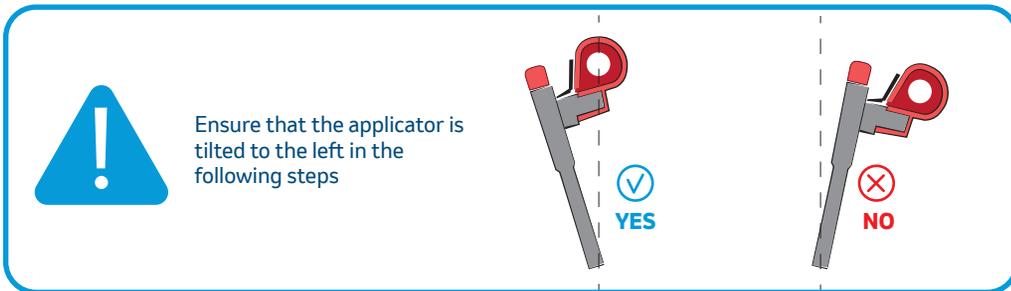

7  
Pull topslide back to cut the tag.

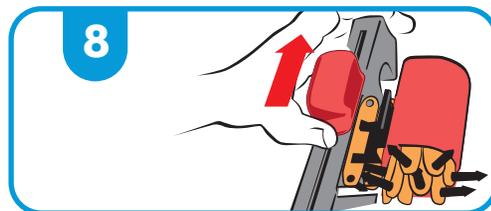

8  
Push topslide forward to load into applicator jaw.

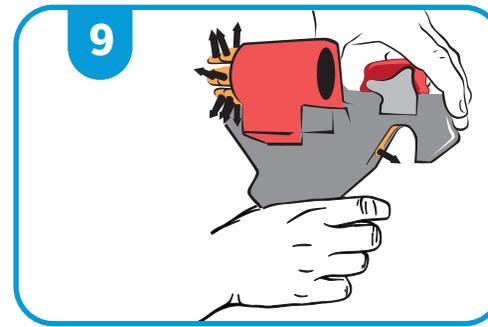


9  
Check tag position.



10  
Avoid Iodine based disinfectants when sterilising tags. If irritation occurs after applying the identification tag, please consult your veterinarian for appropriate treatment.



11  
Select optimum position on ear for tag. Pull trigger to apply.

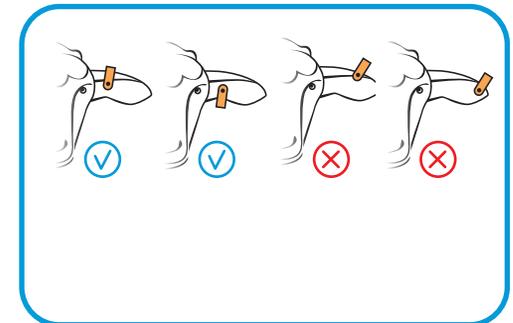

Tags should be located as close to the head as practically possible, allowing room for growth if required.

